



DIGIMICRO

MF-1001

User's Manual

Thank you for purchasing the Nikon DIGIMICRO MF-1001.



Read thoroughly this user's manual before starting operation to be sure of getting optimum performance and longer service life from the unit.

- Reproduction of the contents of this manual, in whole or in part, without permission of Nikon is prohibited.
- The information contained in this manual is subject to change without notice.
- This manual has been prepared with great care. If you have any questions or comments, or find any errors, please contact your local Nikon representative.
- When you use the product in combination with peripheral devices, read the relevant user's manuals.
- This manual and the Nikon product(s) (hereinafter "the product(s)"), including technologies and software, described in this manual are under export restriction. The export of this manual and the product is controlled by the Japanese Foreign Exchange and Foreign Trade Act and international export control regimes. They shall not be exported without authorization from the appropriate governmental authorities.

About WARNING and CAUTION symbols used in the manual

Nikon products are designed with full consideration of safety. However, improper use or failure to observe precautions may result in injury or damage to property. Thoroughly read this user's manual before you use the product, and use the product appropriately. We recommend that you download or bookmark the manual so that you can refer to it whenever necessary.

This manual uses the following symbols to highlight what requires special attention for safety. Be sure to follow the instructions with those symbols.

Symbol	Description
 WARNING	Failure to follow the instructions may result in death or a serious injury.
 CAUTION	Failure to follow the instructions may result in injury or property damage.

 **WARNING****1. Purpose of Using the Product**

This product is precision measuring equipment. Do not use the product for any purposes other than its intended use.

2. Do Not Disassemble or Modify

Do not disassemble or modify the product. Such actions may cause a malfunction and/or electrical shock. If you notice an abnormality, contact your local Nikon representative.

3. Do Not Splash Water or Allow Foreign Matter to Enter the Product

To prevent the product from a failure or abnormal heat generated by a short circuit, never wet the product or any devices used with it or allow them to be contaminated by foreign matter. If they should get wet or foreign matter such as a piece of paper should get inside the product or peripheral devices, immediately turn off their power supplies, and then remove the AC power cord of the AC adapter. Avoid operating the product in this condition and contact your local Nikon representative.

4. Do Not Excessively Bend or Twist the Cables

Do not excessively bend or twist the cables. Such actions may damage the cables, causing an ignition or fire.

 **CAUTION****1. Turn the Power of the Peripheral Devices OFF before Installation or Cable Connection/ Disconnection**

To prevent any failure or malfunction, always turn off the power of the peripheral devices when installing the product or connecting or removing the cables.

2. Precautions for Installation and Storage

- Be careful not to get your fingers or hands pinched.
- This product is precision equipment. In order to prevent any failure and maintain accuracy, always handle the product with sufficient care and avoid applying a shock or strong vibrations.
- If the product is not to be used for a long time, turn off the power switches of the peripheral devices and remove the AC power cord of the AC adapter from the outlet.

Notes on the use of the product

Handle with care

- This product is precision measuring equipment. Handle the product carefully to avoid applying excessive force or shock.
- To make a continuous measurement with the product connected to an automated machine, secure the tip of the spindle to the surface to be measured, where care should be taken not to allow radial load in excess of the specified value to apply to the spindle.
- Avoid tracing the surface to be measured with the use of only measuring force generated by the product.
- Contaminated spindle may cause a malfunction. Wipe the dirty spindle with a dry cloth.

Installation

Install the product in a stable, vibration-free place. Do not install the product near direct sunlight, in an excessively dusty environment, or in a place subject to extreme temperature change. Do not use the product in an environment that exceeds the operating temperature range (0°C to 40°C).

Disposal

When disposing of the product, follow the laws and regulations of your country or region.

Table of Contents

About WARNING and CAUTION symbols used in the manual	ii
⚠ WARNING	iii
⚠ CAUTION	iii
Notes on the use of the product.....	iv



1	Names and Functions of Components	1
2	System Configuration	2
2.1	Configuration of DIGIMICRO Series	2
2.2	Configuration example	2
3	How to Use the DIGIMICRO	3
3.1	Example of general measurement	3
3.2	Direction of measurement.....	4
3.3	Probe.....	4
3.4	To reduce measuring force.....	4
4	Options	5
5	Troubleshooting.....	6
6	Performance and Specifications.....	7
7	Output Connector	9
8	Accessories	9
9	Repair.....	10
10	Contact information	10

1 Names and Functions of Components

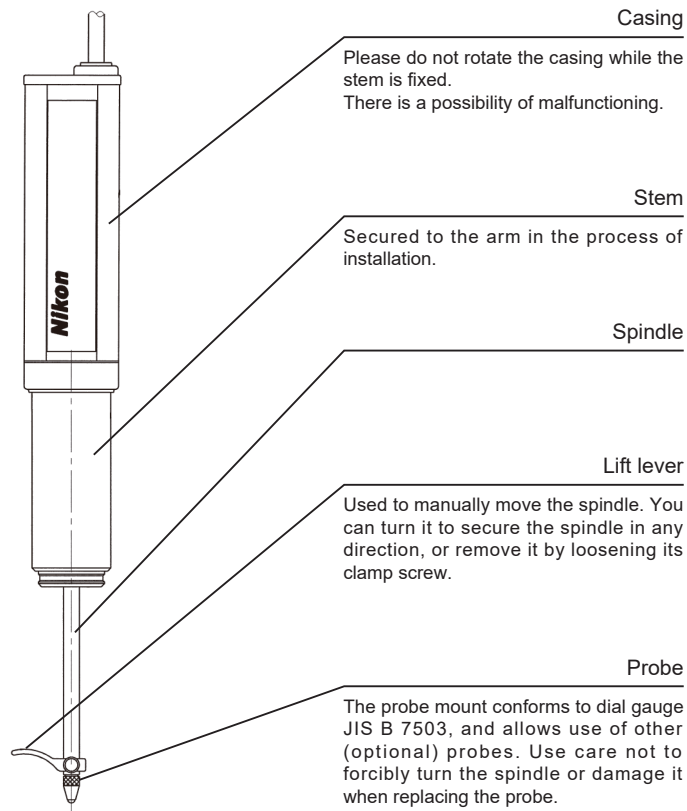


Figure 1 Component names


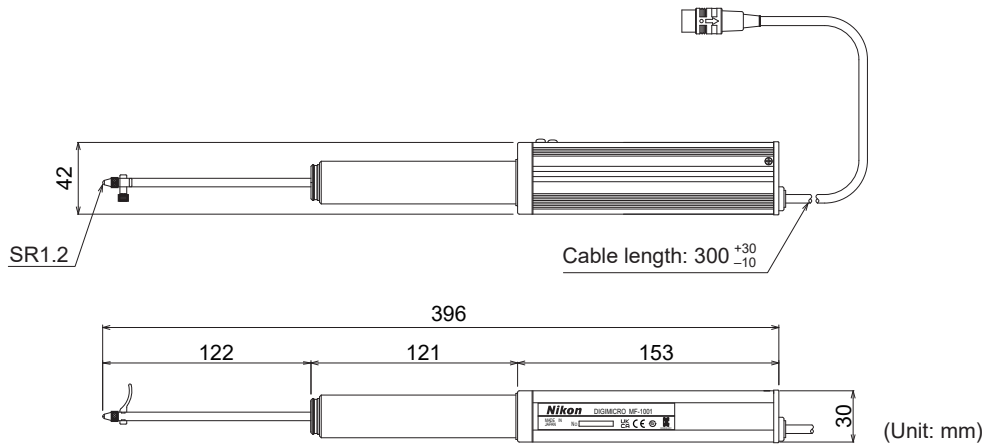


Figure 2 Outline dimensions

2 System Configuration

2.1 Configuration of DIGIMICRO Series

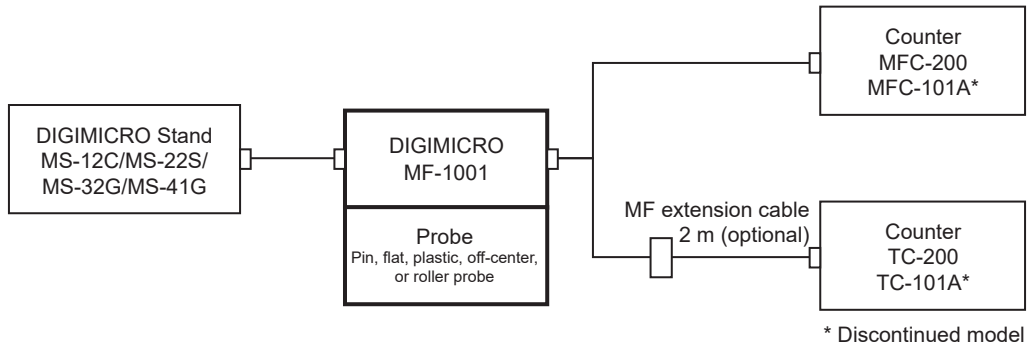

Note:

- Counters, DIGIMICRO Stands, probes, and cables other than the standard probe are optional. To purchase optional components, contact your local Nikon representative from which you purchased the DIGIMICRO. For details about connection with other devices, contact your local Nikon representative as well.

Figure 3

2.2 Configuration example

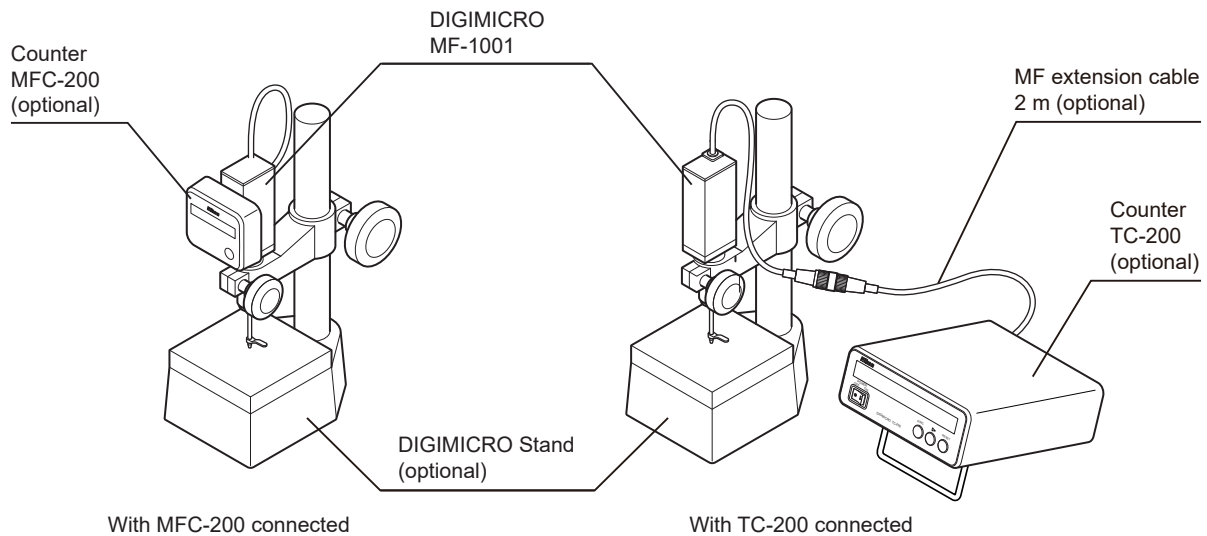


Figure 4 With the Counter connected

3 How to Use the DIGIMICRO

3.1 Example of general measurement

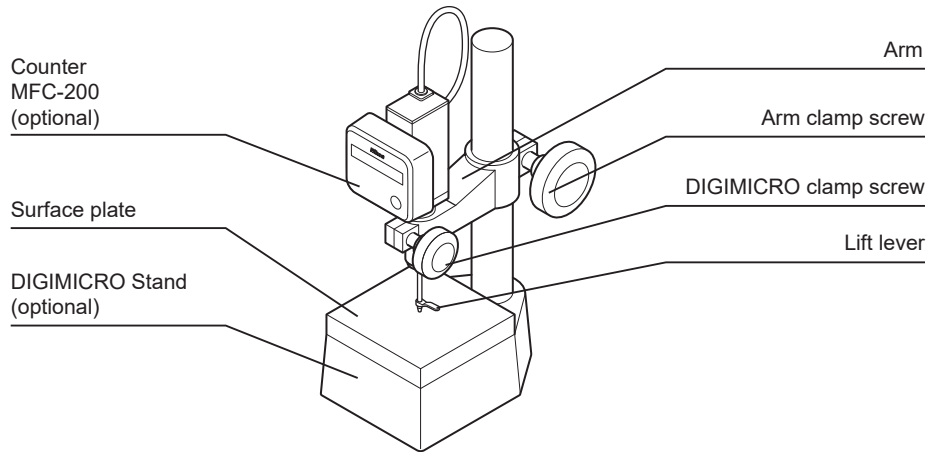


Figure 5 With the DIGIMICRO MF-1001 and Counter MFC-200 (optional) mounted to the DIGIMICRO Stand (optional)

(1) Securing the DIGIMICRO



CAUTION

- When securing the DIGIMICRO, see the DIGIMICRO Stand user's manual.
- Do not exert excessive force when tightening the stem. Overtightening might cause a failure such as impaired spindle operation.
- Do not tighten the arm clamp screw without the DIGIMICRO installed. Failure to follow this instruction might cause a failure in the DIGIMICRO Stand and the product.

Secure the stem of the DIGIMICRO to the arm by tightening the clamp screw.

Before measuring, be sure to secure the stem to the arm.

(2) Moving the DIGIMICRO



CAUTION

- Always tighten the arm clamp screw with the arm supported. The DIGIMICRO may fall together with the arm unless you support the arm.

Move the DIGIMICRO together with the arm until the probe comes into contact with the surface plate on the DIGIMICRO Stand and secure the DIGIMICRO by tightening the arm clamp screw.

(3) Turning off the power supply

Turn off the power supply of the connected devices.

The product does not have a power supply. For details about how to operate the power supply of the connected devices, see the relevant user's manual.

(4) Zero reset

To reset the DIGIMICRO to zero, press the Reset switch of the DIGIMICRO Counter (optional) with the probe held against the surface plate.

For details about how to perform zero reset, see the user's manual of the Counter (optional).

(5) Turning on the power supply

Turn on the power supply of the connected devices.

The product does not have a power supply. For details about how to operate the power supply of the connected devices, see the relevant user's manual.

(6) Measurement

Notes:

- To assure accurate measurement, avoid applying excessive shock on the end of the probe.
- If the spindle is moved too quickly, an overspeed error occurs.
- Not taking into consideration factors such as temperature and dust in the air may lead to unforeseen measurement errors.
- When conducting a high-precision measurement of a mirrored plane surface like a block gauge, prepare a reference plane made from the same materials and with the same surface state. Thoroughly clean this reference plane and the measuring object surface and then bring them into close contact (linking) to carry out measurement.

Raise the spindle by holding the hook on the lift lever with your hand, put a piece to be measured under the spindle, and then slowly lower the spindle until the probe comes into contact with the surface to be measured.

3.2 Direction of measurement

The spindle movement can be set to lateral or downward direction. Note that the measuring force varies with the direction and spindle position.

3.3 Probe

The probe is replaceable with other probes that conform to dial gauge JIS B 7503.

3.4 To reduce measuring force

When the product is only used in a downward direction, it is possible to modify the product so that the measuring force is reduced to approximately 0.44 N. If you require this modification, please contact your local Nikon representative.

4 Options

Options shown in Figure 3 and Figure 4 are available.

- Probes (optional)

Probes shown in Figure 6 are available in addition to the standard probe.

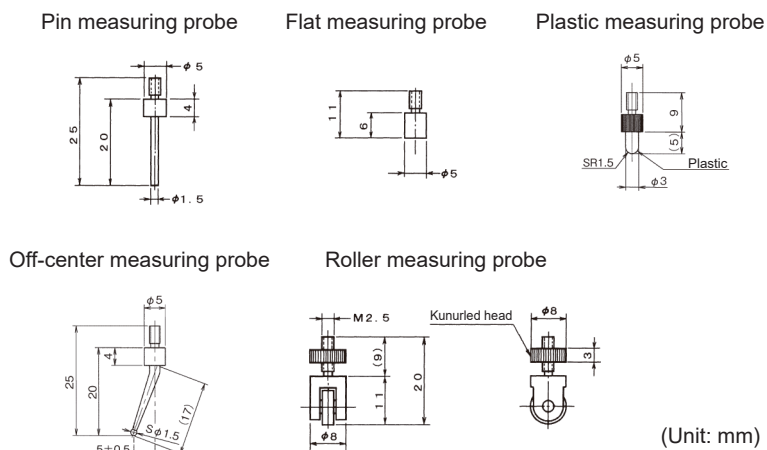


Figure 6

- DIGIMICRO Stand (optional)

	Maximum measuring height	Size of surface plate
MS-12C	Approx. 150 mm	111 mm x 111 mm
MS-22S	Approx. 200 mm	150 mm x 150 mm
MS-32G	Approx. 170 mm	120 mm x 180 mm
MS-41G	Approx. 290 mm	400 mm x 300 mm

- Counter (optional)

MFC-200

TC-200

- Extension cable (optional)

MF extension cable (2 m)

5 Troubleshooting

Should the product fail to operate properly, locate a possible cause of the trouble by referring to the table below.

Table 1

Trouble	Check to see if:
<ul style="list-style-type: none"> • Spindle binds. • The motion of spindle suddenly becomes stiff. 	<ul style="list-style-type: none"> • Spindle is not dirty. • Excessive radial load is not applied to the spindle. • The stem has not been overtightened.
<ul style="list-style-type: none"> • Measurement error • Bad repeatability 	<ul style="list-style-type: none"> • The measuring probe is securely installed. • The stem is securely installed. • The DIGIMICRO, DIGIMICRO Stand, and other components are installed properly. • Excessive load is not applied to the DIGIMICRO.
<ul style="list-style-type: none"> • Faulty counting • A message. "Error X", appears frequently. 	<ul style="list-style-type: none"> • Power switch of the Counter is turned on. • The DIGIMICRO and Counter are properly connected. • Travel speed is appropriate. • There are no sources generating noise in the vicinity of the product. • The cable is not defective. • The dedicated AC adapter for the DIGIMICRO Counter in use is used.

6 Performance and Specifications

Recommended minimum reading	: 0.1 μm
Measuring range	: 100 mm
Accuracy	: 3 μm at 20°C
Response speed (at 0.1 μm resolution)	: Max. 500 mm/s
Measuring direction	: Any direction
Measuring force	: Downward 1.23 to 1.81 N (Modifiable to approx. 0.44 N. Contact your local Nikon representative from which you purchased the DIGIMICRO.) Lateral 0.64 to 1.23 N
Weight	: 0.48 kg
Allowable spindle load	: Radial 0.98 N (100 gf) Twisting moment (4.9 mN•m)
Probe	: Probe conforming to dial gauge JIS B 7503
Temperature	: 0 to 40°C in use -20 to 60°C in storage
Conforming standards	: CE



EMC Directive
RoHS Directive

This product conforms to EN standards and shows the CE Marking.

This product has been tested and found to comply with the limits for a Class A device, pursuant to EMC DIRECTIVE. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This product must not be used in residential areas.

KC



사용자안내문

이 기기는 업무용 환경에서 사용할 목적으로 적합성평가를 받은 기기로서 가정용 환경에서 사용하는 경우 전파간섭의 우려가 있습니다.

WEEE



This symbol indicates that this product is to be collected separately.

The following apply only to users in European countries.

- This product is designated for separate collection at an appropriate collection point. Do not dispose of as household waste.
- For more information, contact the retailer or the local authorities in charge of waste management.

UKCA



FCC



This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

CAN ICES-3 (A)/NMB-3 (A)

7 Output Connector

- Model: RP17A-13P-12PC (manufacturer: Hirose Electric Co., Ltd.)
12-pin circular connector (plug)
- Matching connector: RP17A-13RA-12SD (manufacturer: Hirose Electric Co., Ltd.) (receptacle)

Table 2 Pin assignment and signal names

Pin No.	Signal name	Description
1	FG	Frame ground
2	N.C.	Open
3	A	Signal phase A
4	Vref	Signal center level
5	B	Signal phase B
6	Vref	Signal center level
7	N.C.	Open
8	N.C.	Open
9	L+	Power supply for LED
10	0V	0V power supply
11	Vcc	+12V power supply
12	0V	0V power supply

8 Accessories

- Standard probe x 1
- Lift lever x 1
- Safety Precautions x 1
- Product warranty x 1

9 Repair

If you need repair, contact your local Nikon representative.

Repairs covered by the warranty

- A natural failure occurred within the warranty period (one year after the date of purchase), and the product warranty is present.
- After repair, the same part failed in normal handling conditions within six months after the date of return from the previous repair, and the relevant documentation for the previous repair is present.

Any other cases constitute out-of-warranty repairs. Store the product warranty so that it is not lost.

For details, contact your local Nikon representative.

10 Contact information

Table 3 Contact information

Region	Company name	Address	Phone
Japan	NIKON CORPORATION	Shinagawa Intercity Tower C, 2-15-3, Konan, Minato-ku, Tokyo 108-6290, Japan	+81-3-6433-3726
China	NIKON INSTRUMENTS (SHANGHAI) CO., LTD.	1103-1104, Tower 5, Crystal Plaza No. 36, Ping Jia Qiao Road, Pudong New District, Shanghai 200126, China	+86-21-6841-2050
Korea	NIKON INSTRUMENTS KOREA CO., LTD.	21F, City Air Tower, 36, Teheran-ro 87gil, Gangnam-gu, Seoul, 06164, South Korea	+82-2-6288-1900
Europe (Belgium)	NIKON METROLOGY EUROPE NV	Interleuvenlaan 86 3001 Leuven Belgium	+32-16-74-01-01
Europe (UK)	NIKON METROLOGY UK LTD.	Nottingham EMA, Argosy Road Castle Donington Derby DE74 2SA United Kingdom	+44-1332-811-349
USA	NIKON METROLOGY, INC.	12701 Grand River, Brighton Avenue, MI 48116 U.S.A.	+1-810-220-4360

1st Edition

EC16E
April 2022



NIKON CORPORATION

Shinagawa Intercity Tower C, Konan, Minato-ku, Tokyo 108-6290, Japan